

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS ✓
- GRAY SCALE DOCUMENTS

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Problem Image Mailbox.**

Fig. 1

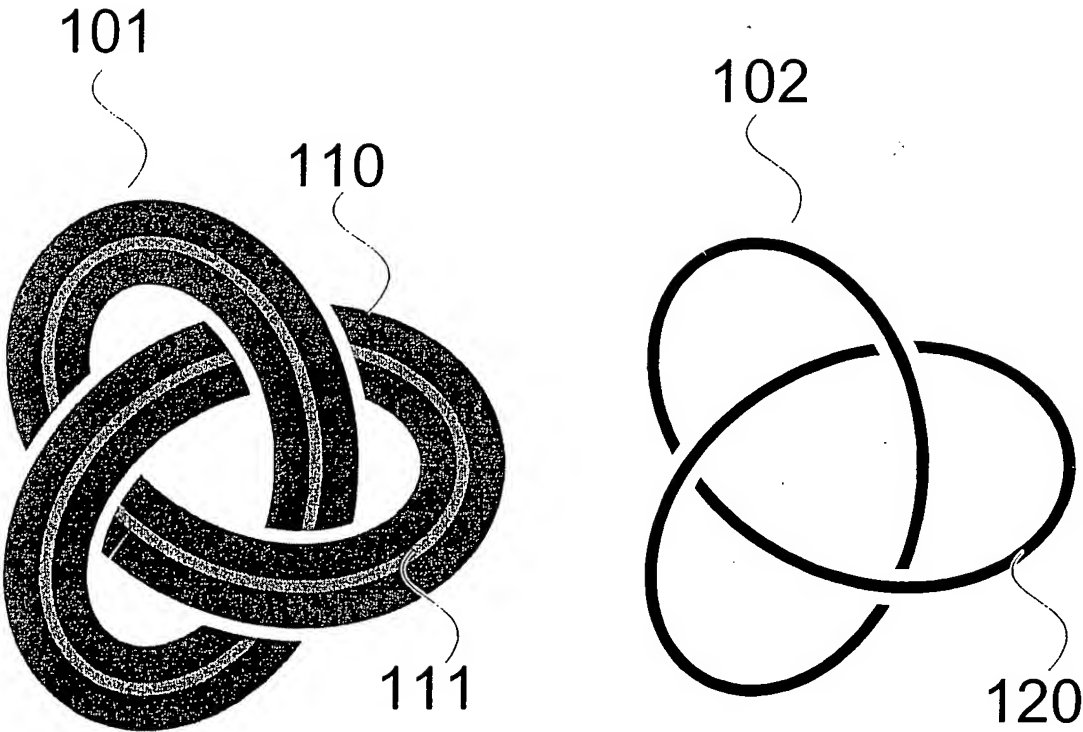


Fig. 2

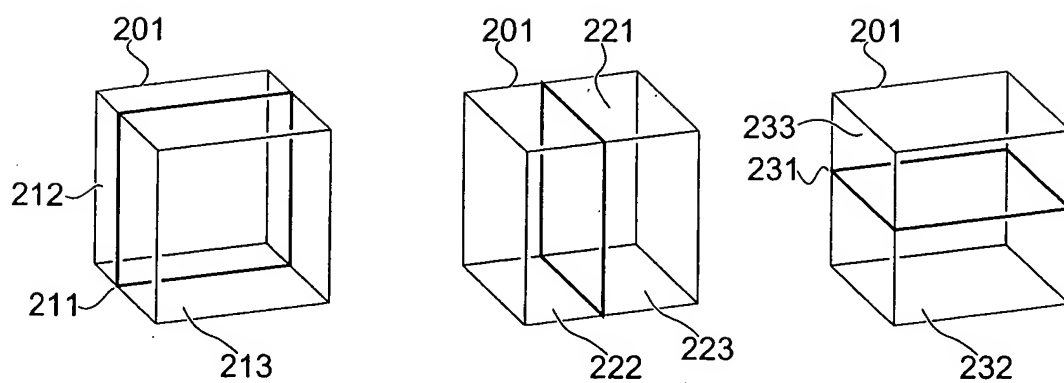


Fig. 3a

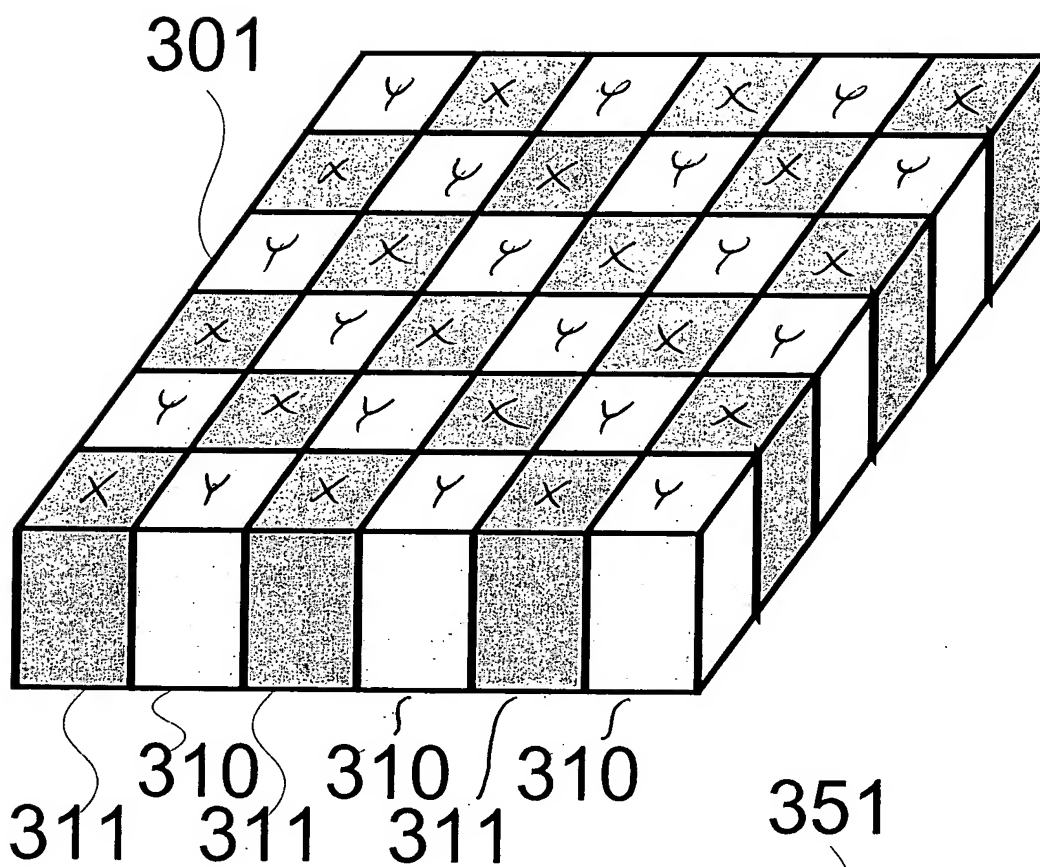


Fig. 3b

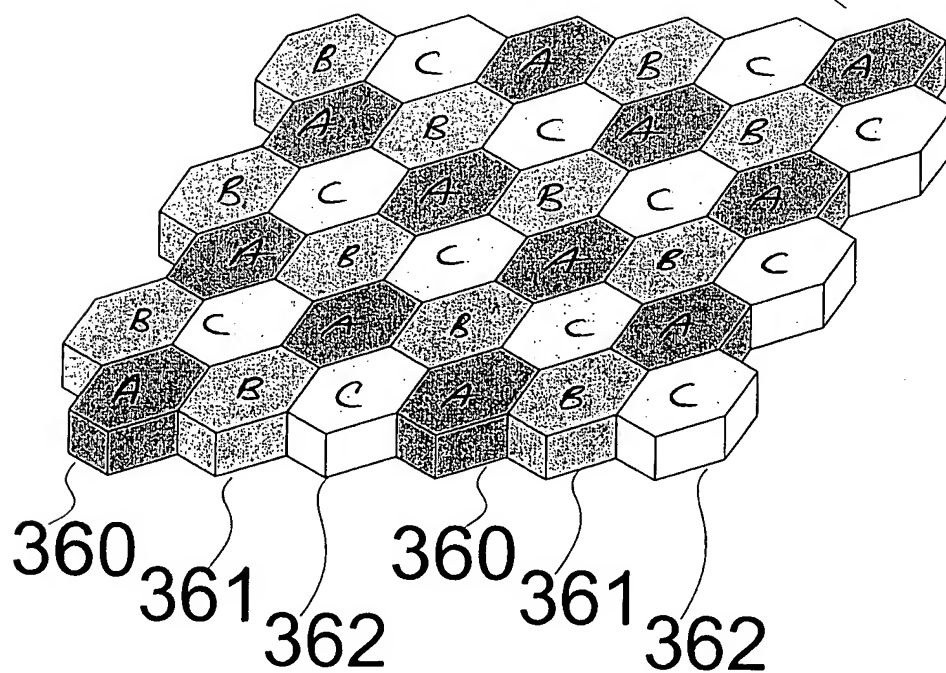


Fig. 4

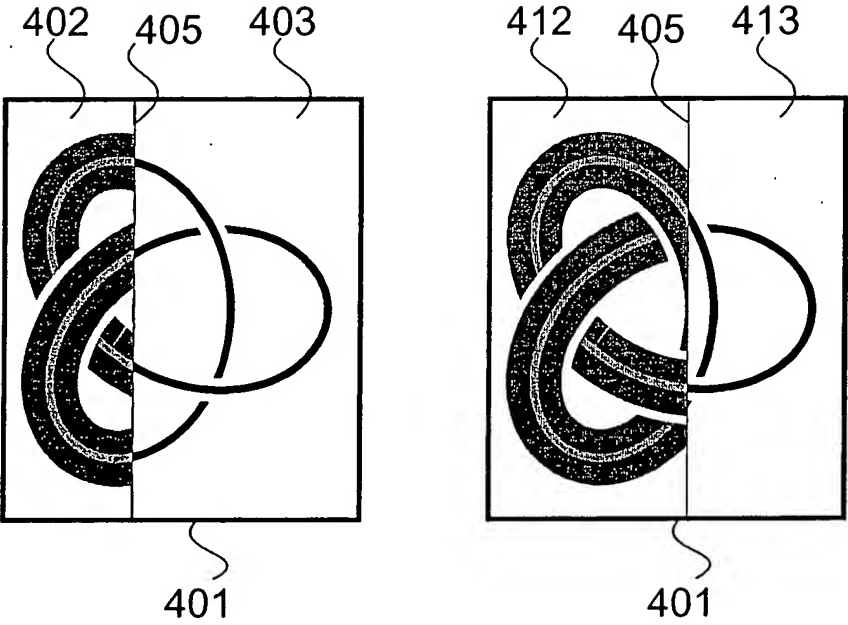


Fig. 5

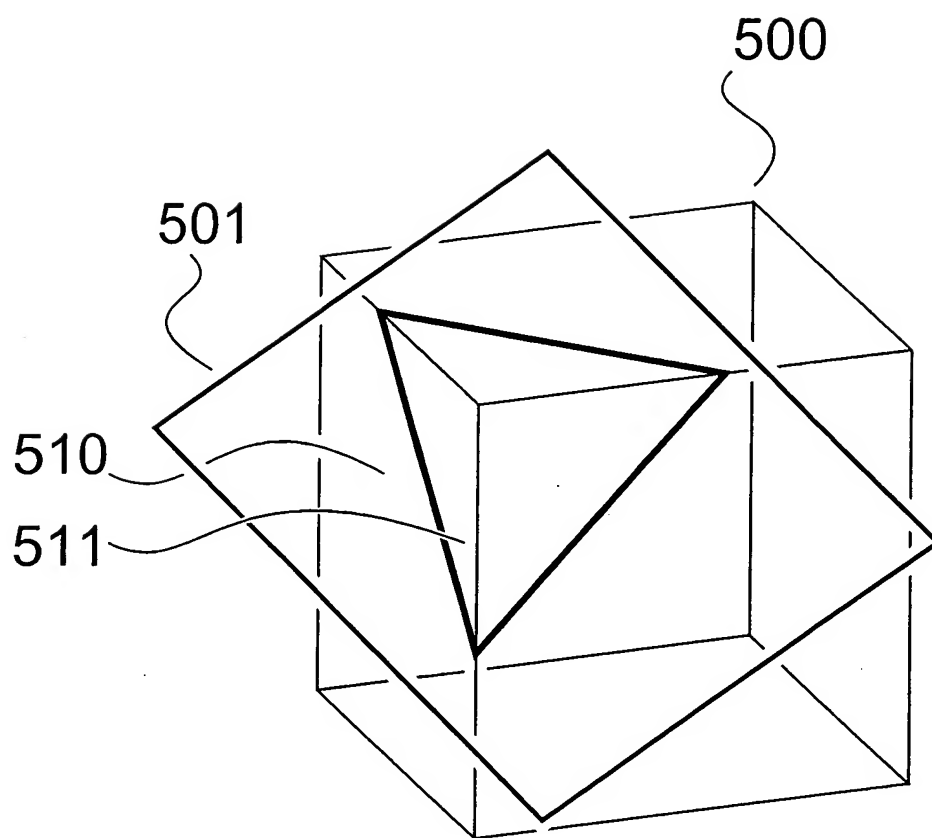


Fig. 6

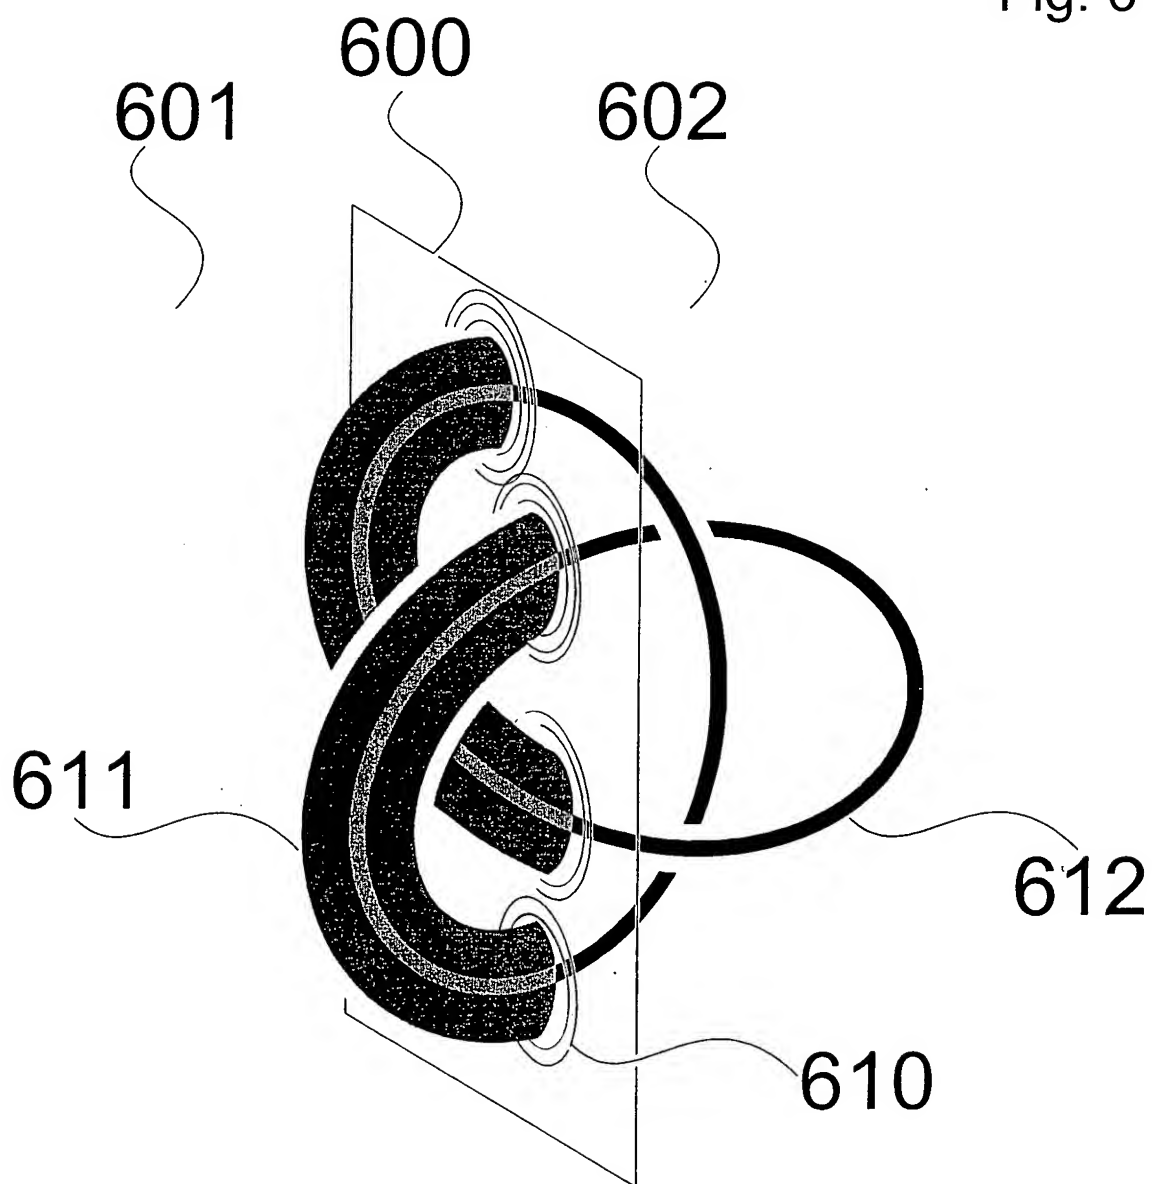


Fig. 7


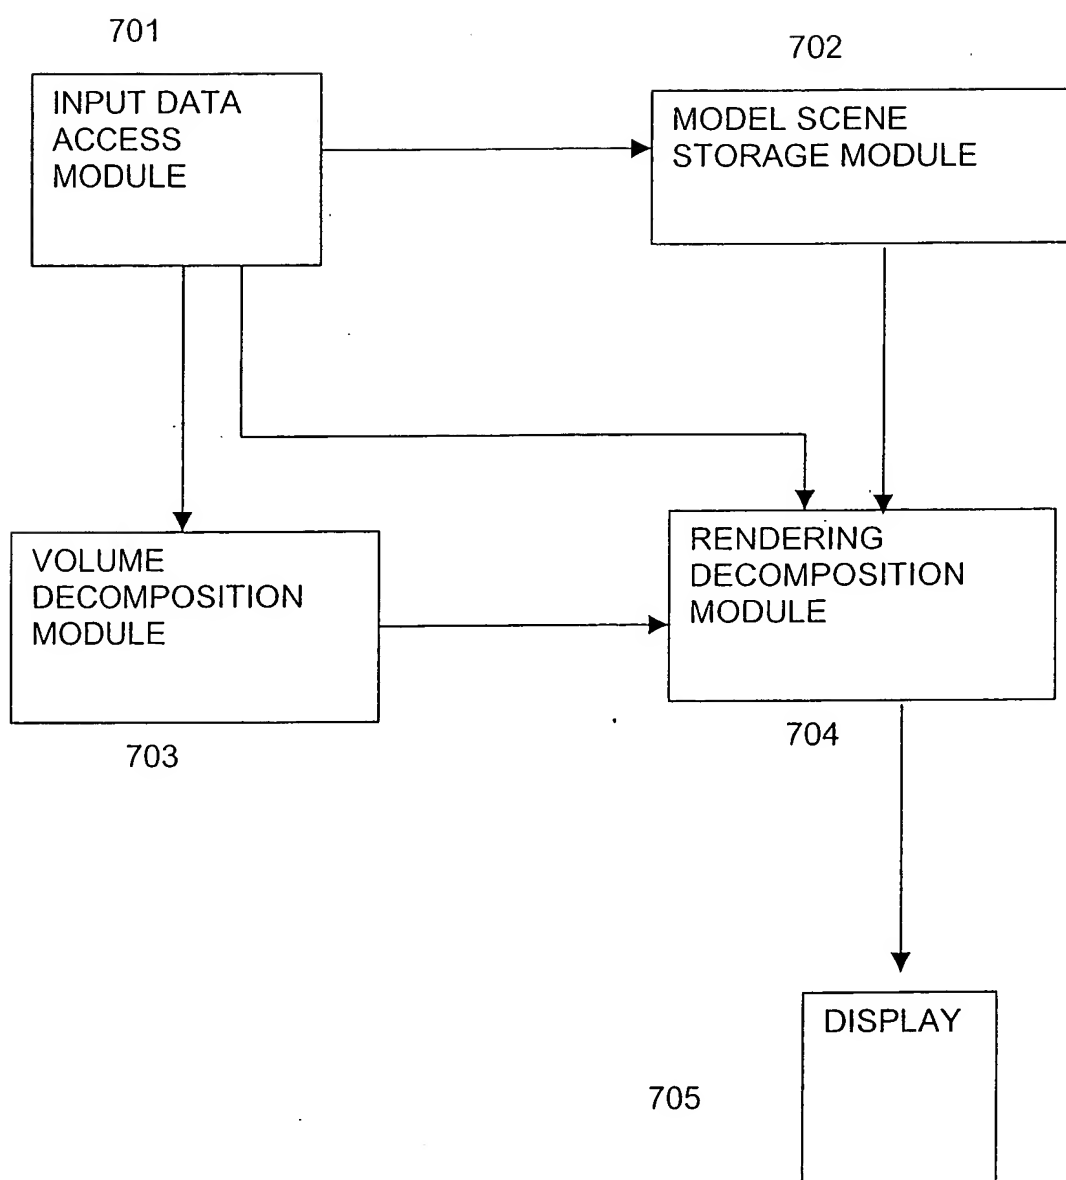


FIG. 8

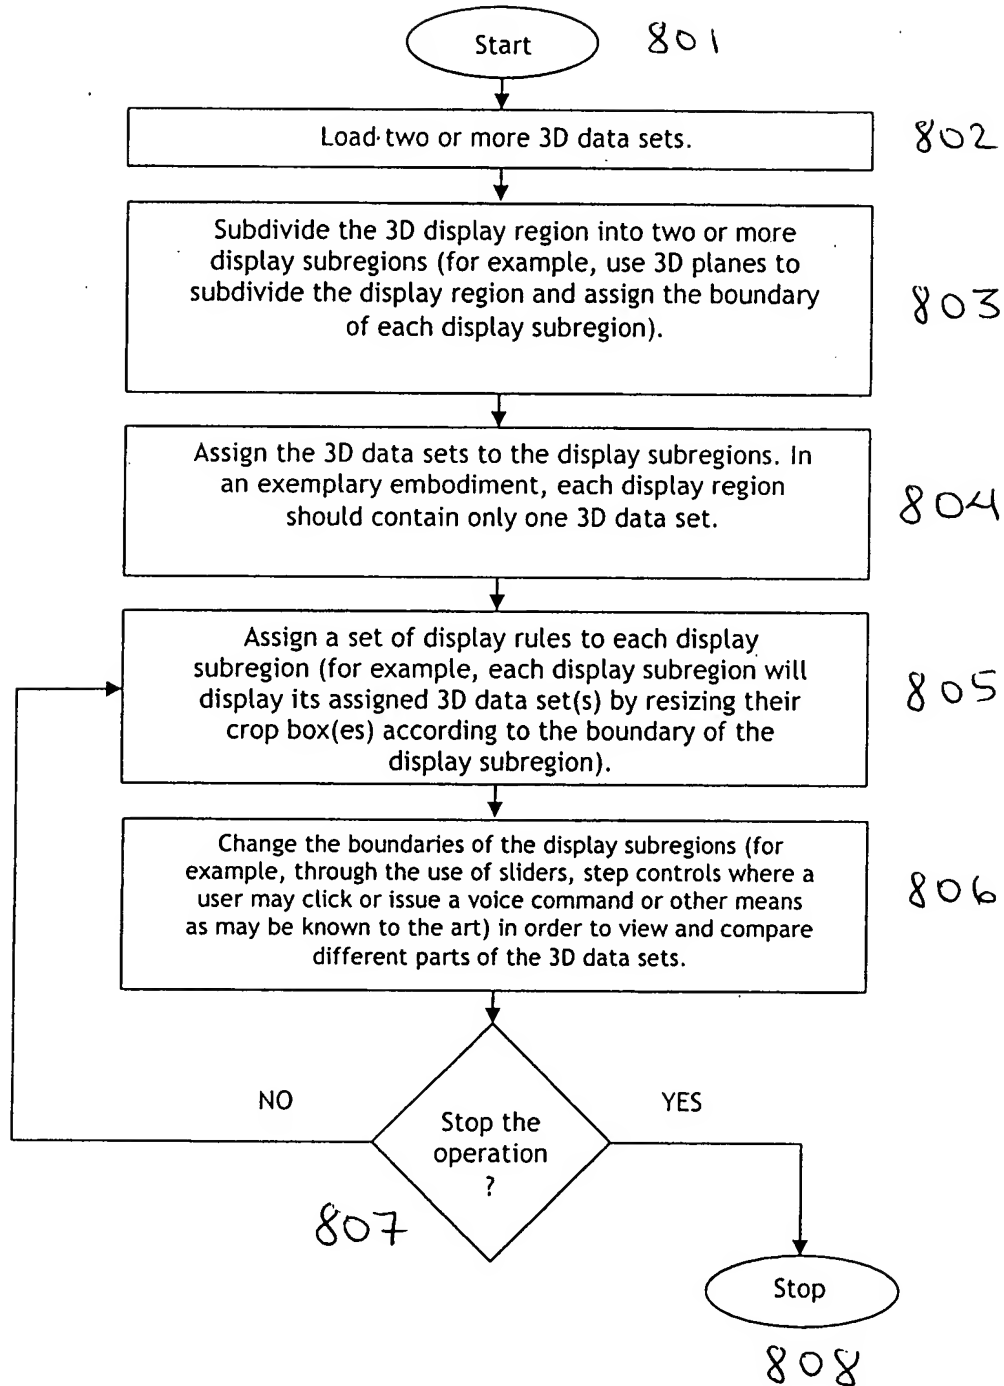

ked object: MRI  
dality:  
e:  
e:  
e: 256x256x52, 3.3MB

120  
100  
80  
60  
40  
20  
0

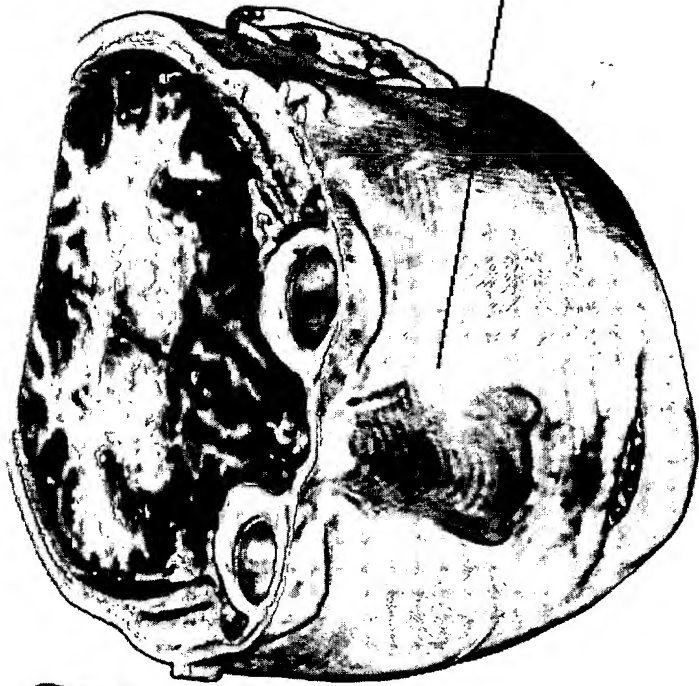
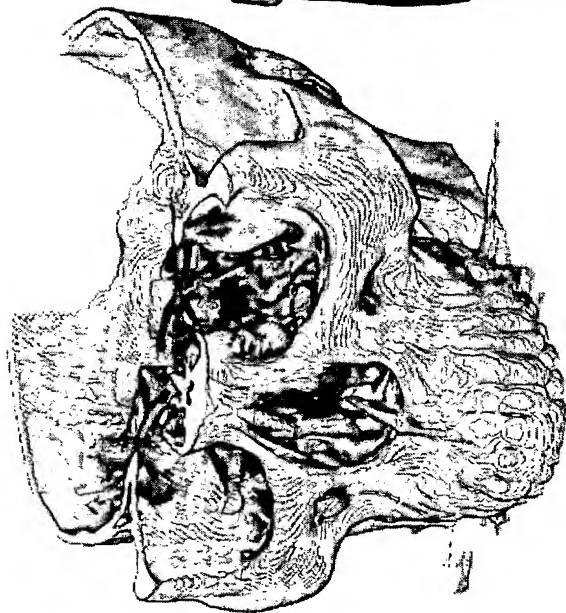


Fig. 9

# Automatic Registrati

ected object: MRI  
dality:  
e:  
e: 256x256x52, 3.3MB


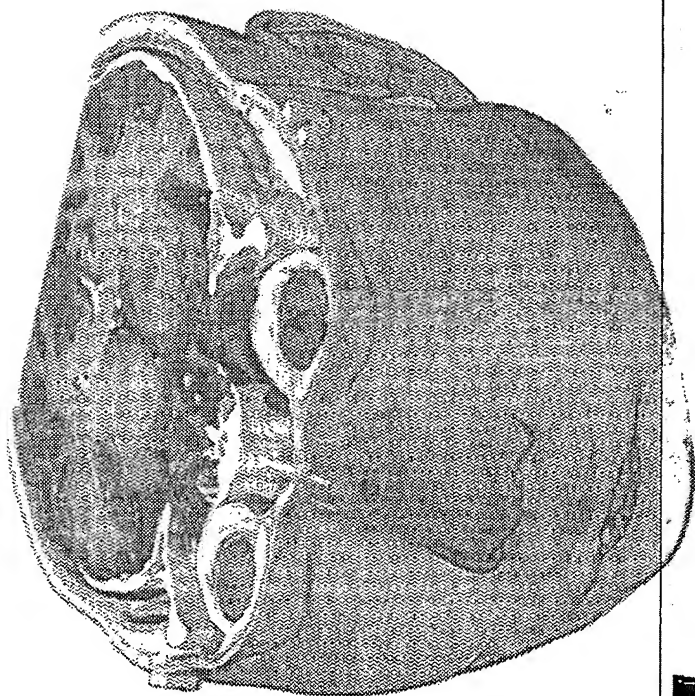


Fig. 10

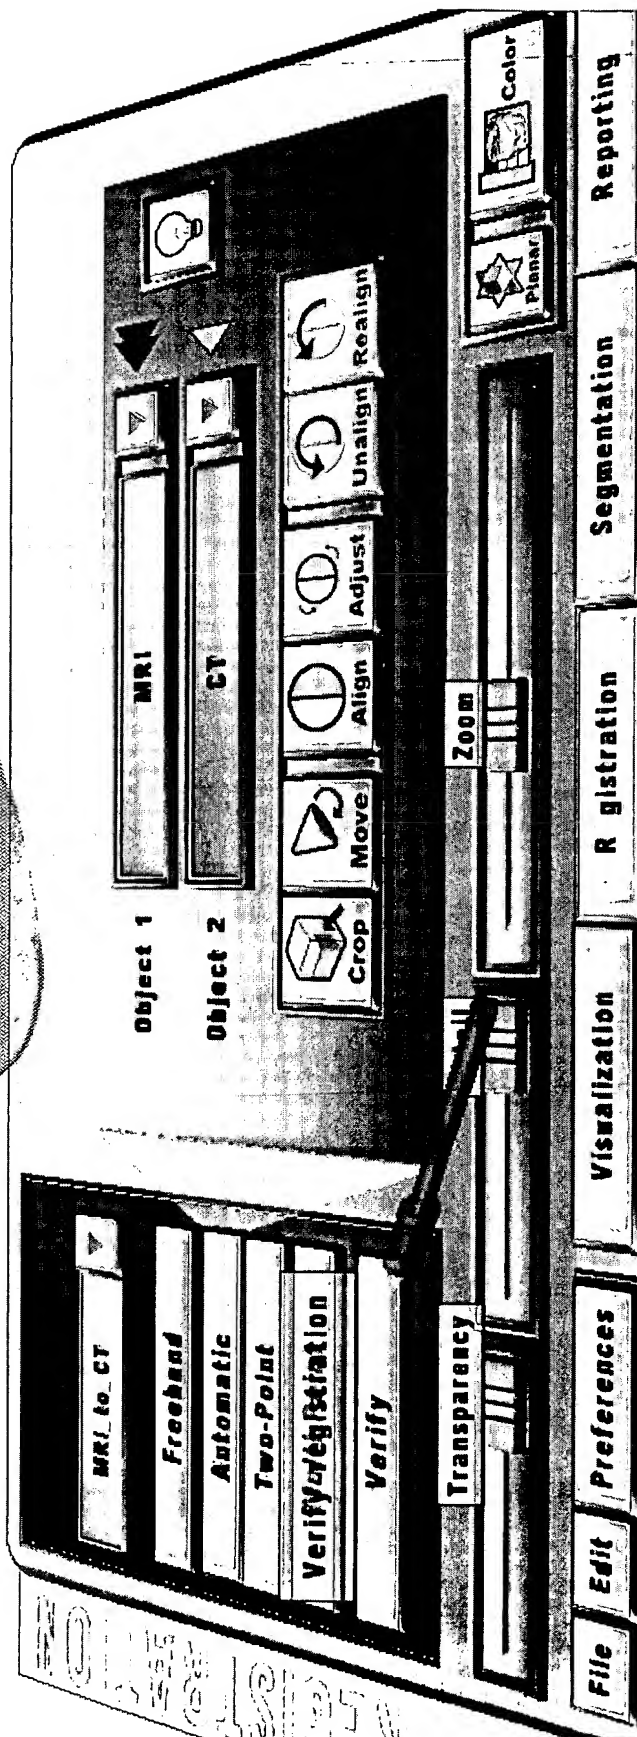

# Verify Registrati

ected object: MRI  
dality:  
e:  
e:  
e: 256x256x52, 3.3MB


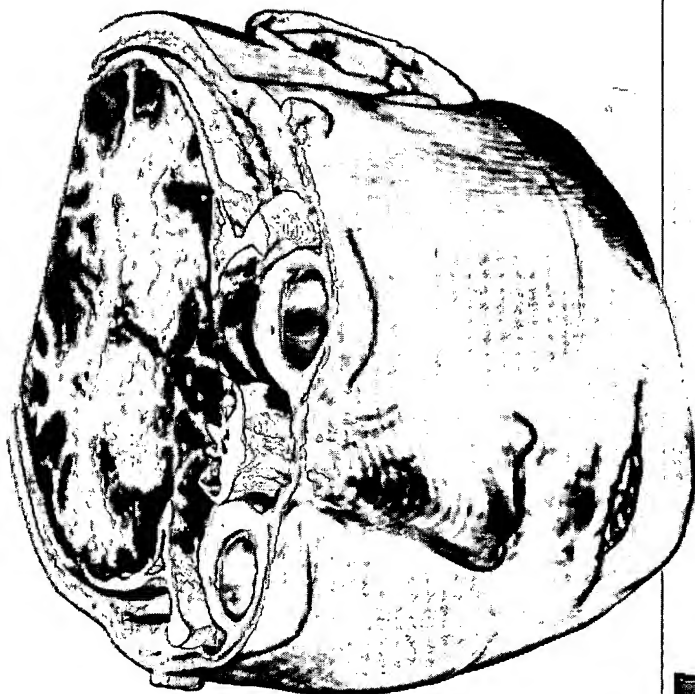


Fig. 11

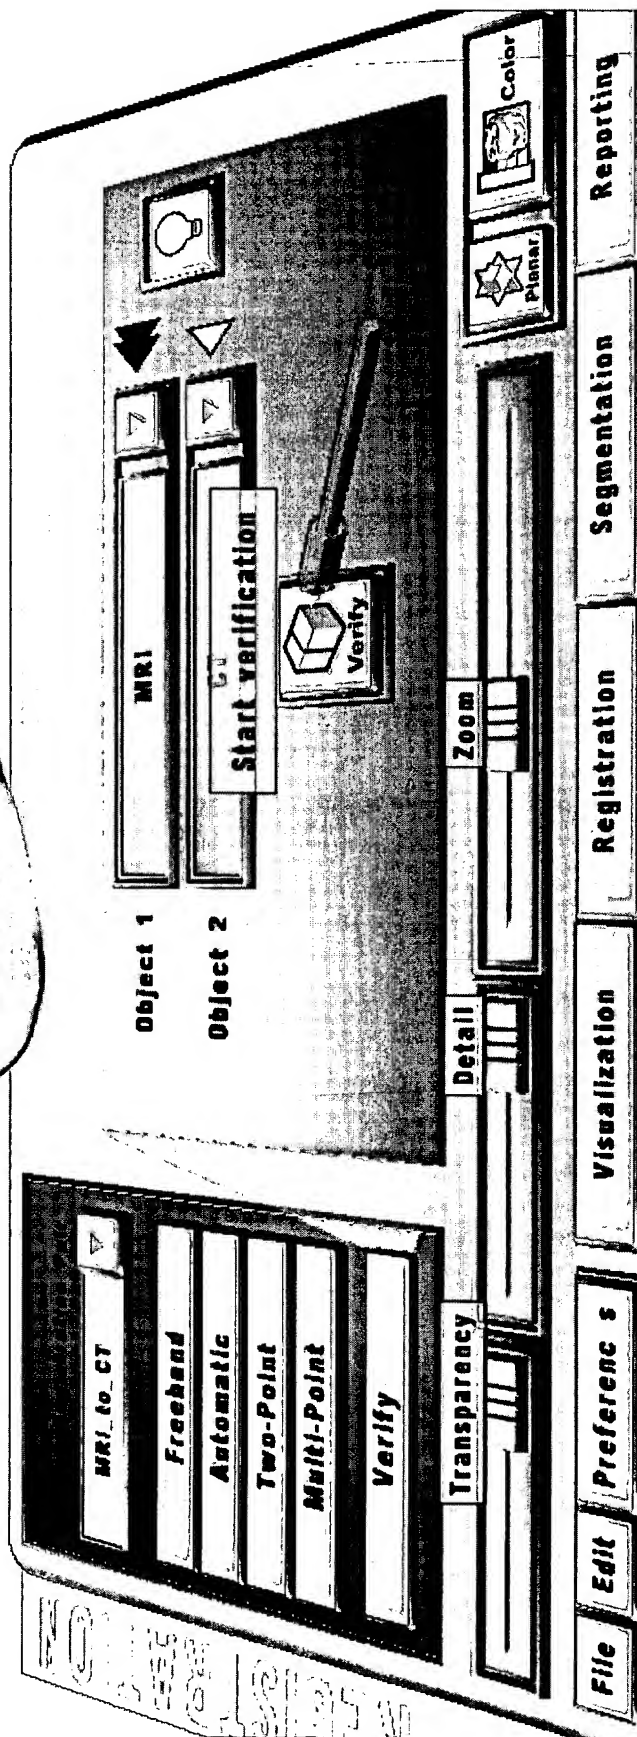

# Verify Registrati

ected object: MRI  
dality:  
e:  
ie:  
e: 256x256x52, 3.3MB

Fig. 12



ected object: MRI

dality:

ie:

ie:

e: 256x256x52, 3.3MB

990  
100  
02  
24  
22  
20  
20  
20  
40  
20  
22  
10  
0

## Verify Registrati

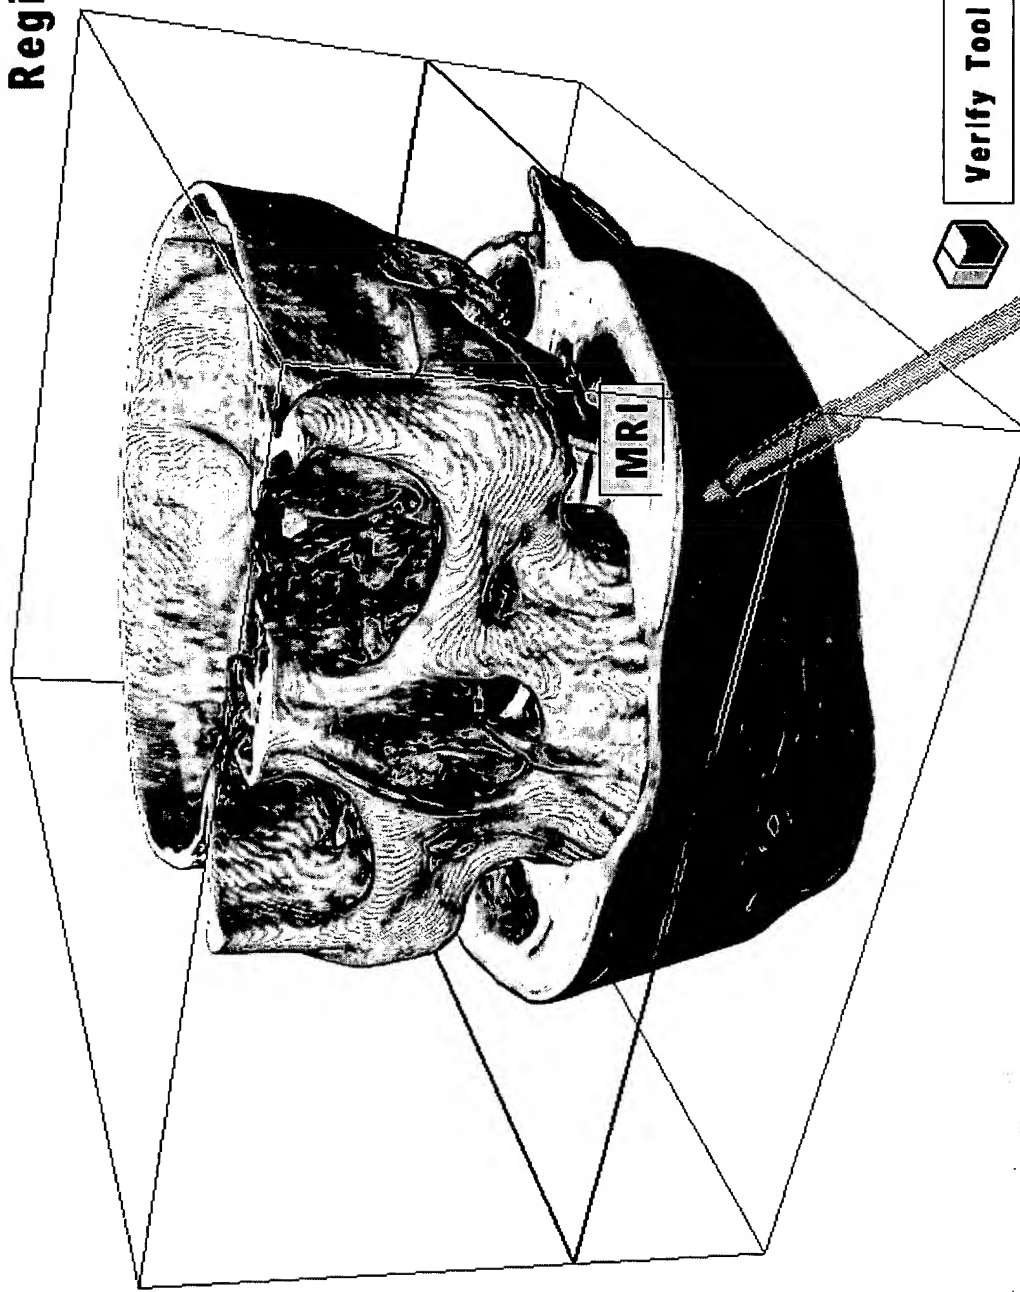


Fig. 13

ected object: MRI


dality:

ie:

ie:

e: 256x256x52, 3.3MB

198  
180  
51  
22  
72  
20  
22  
21  
21  
22  
20  
0



## Verify Registrati

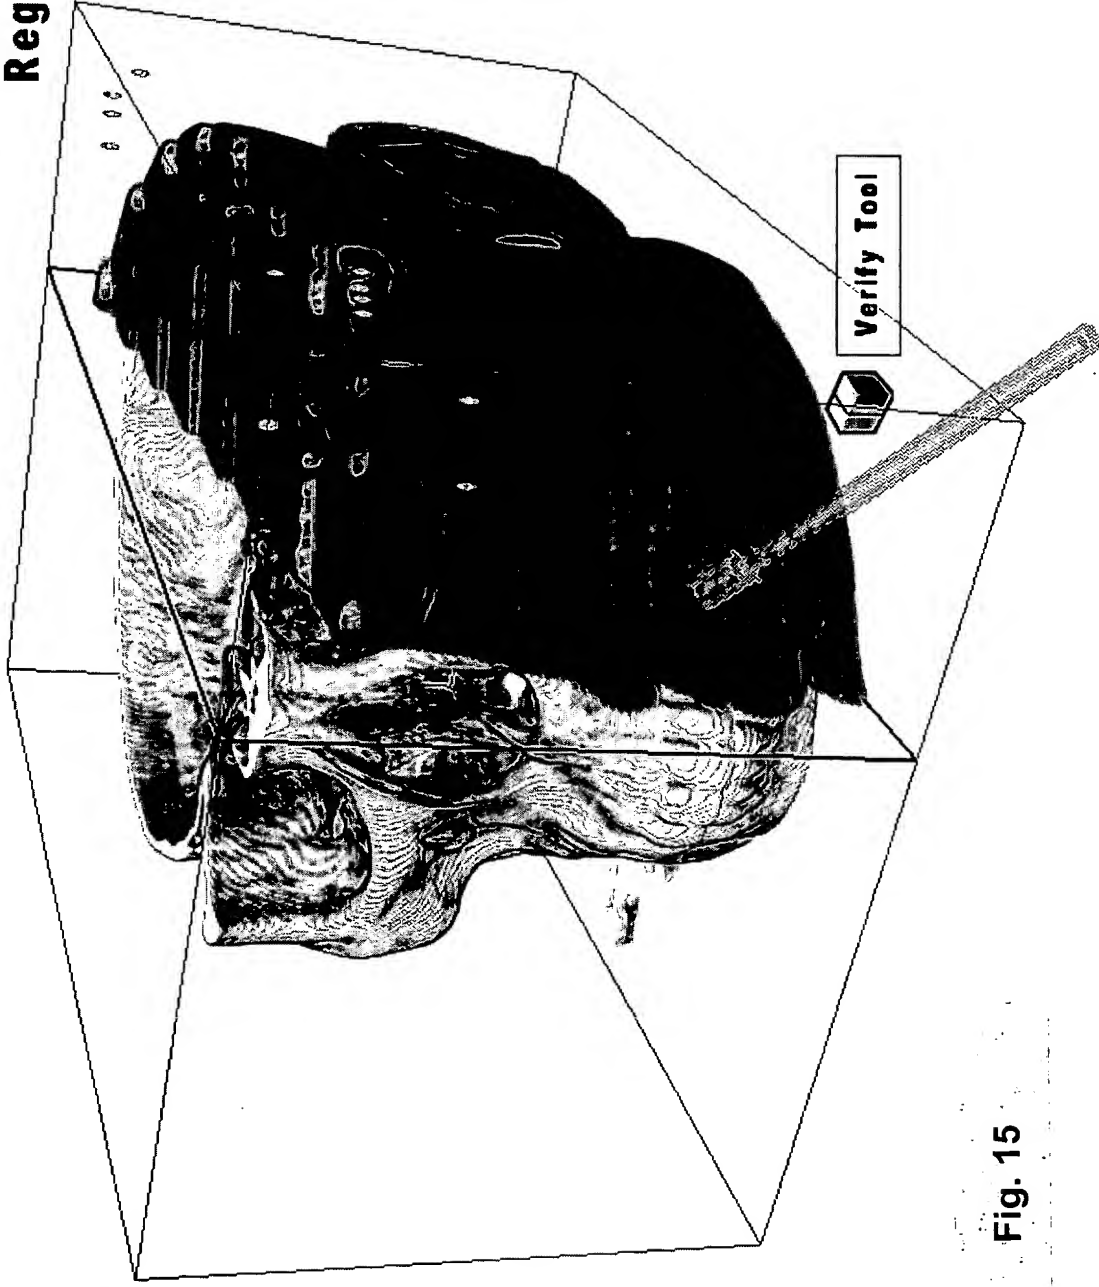


Fig. 15

ected object: MRI

dality:

ie:

ie:

e: 256x256x52, 3.3MB

144  
100  
63  
22  
23  
34  
53  
24  
22  
24  
10  
0

# Verify Registrati

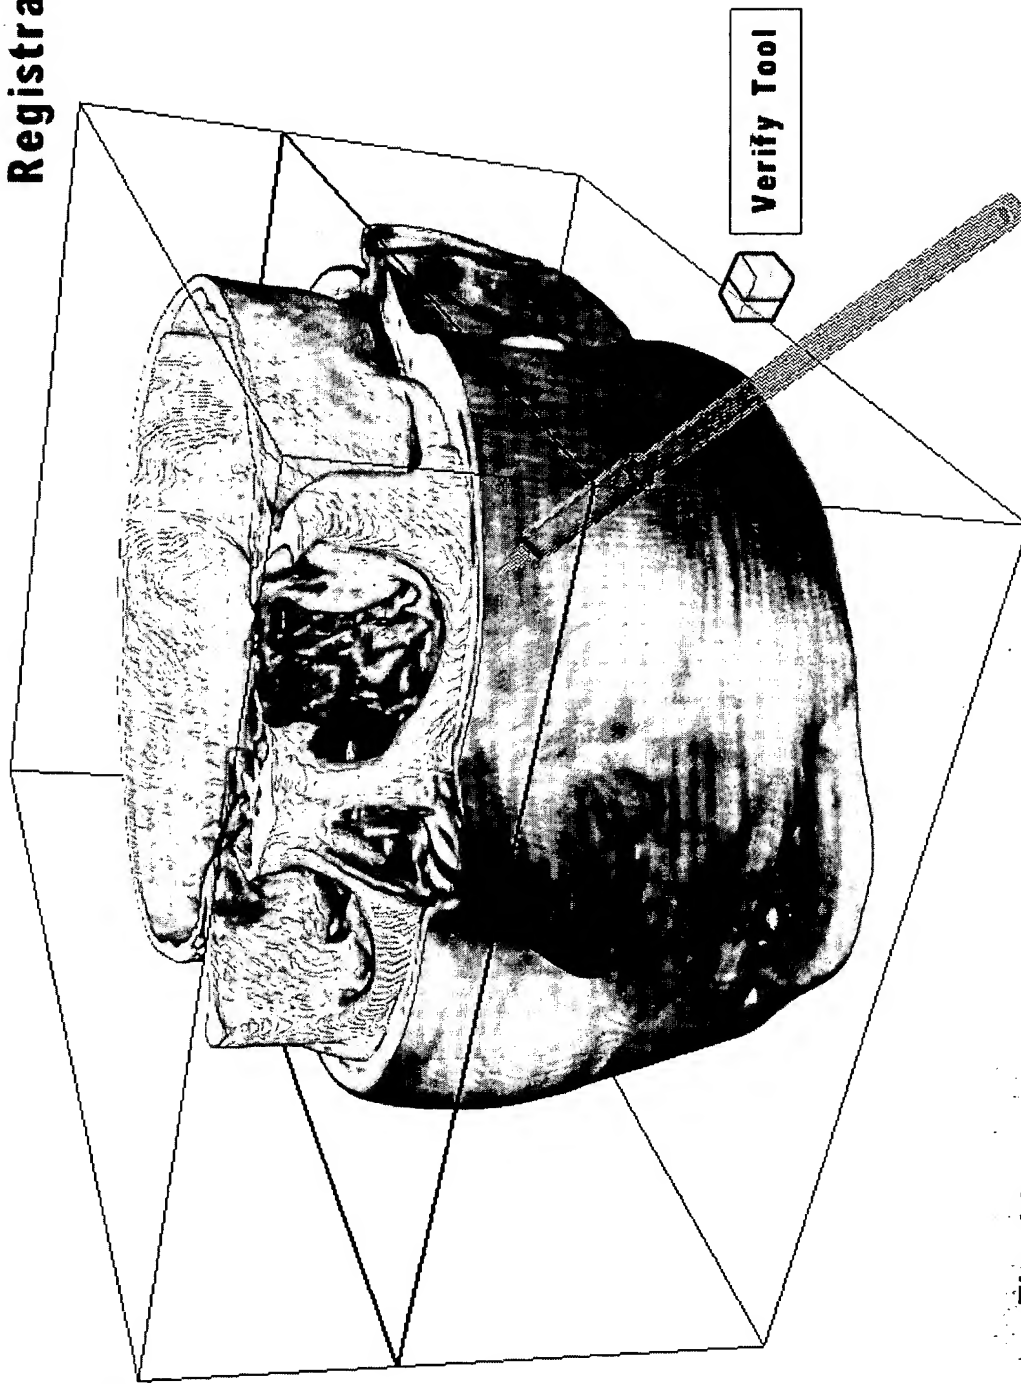


Fig. 14

ected object: MRI

dality:

ie:

ie:

e: 256x256x52, 3.3MB

# Verify Registrati


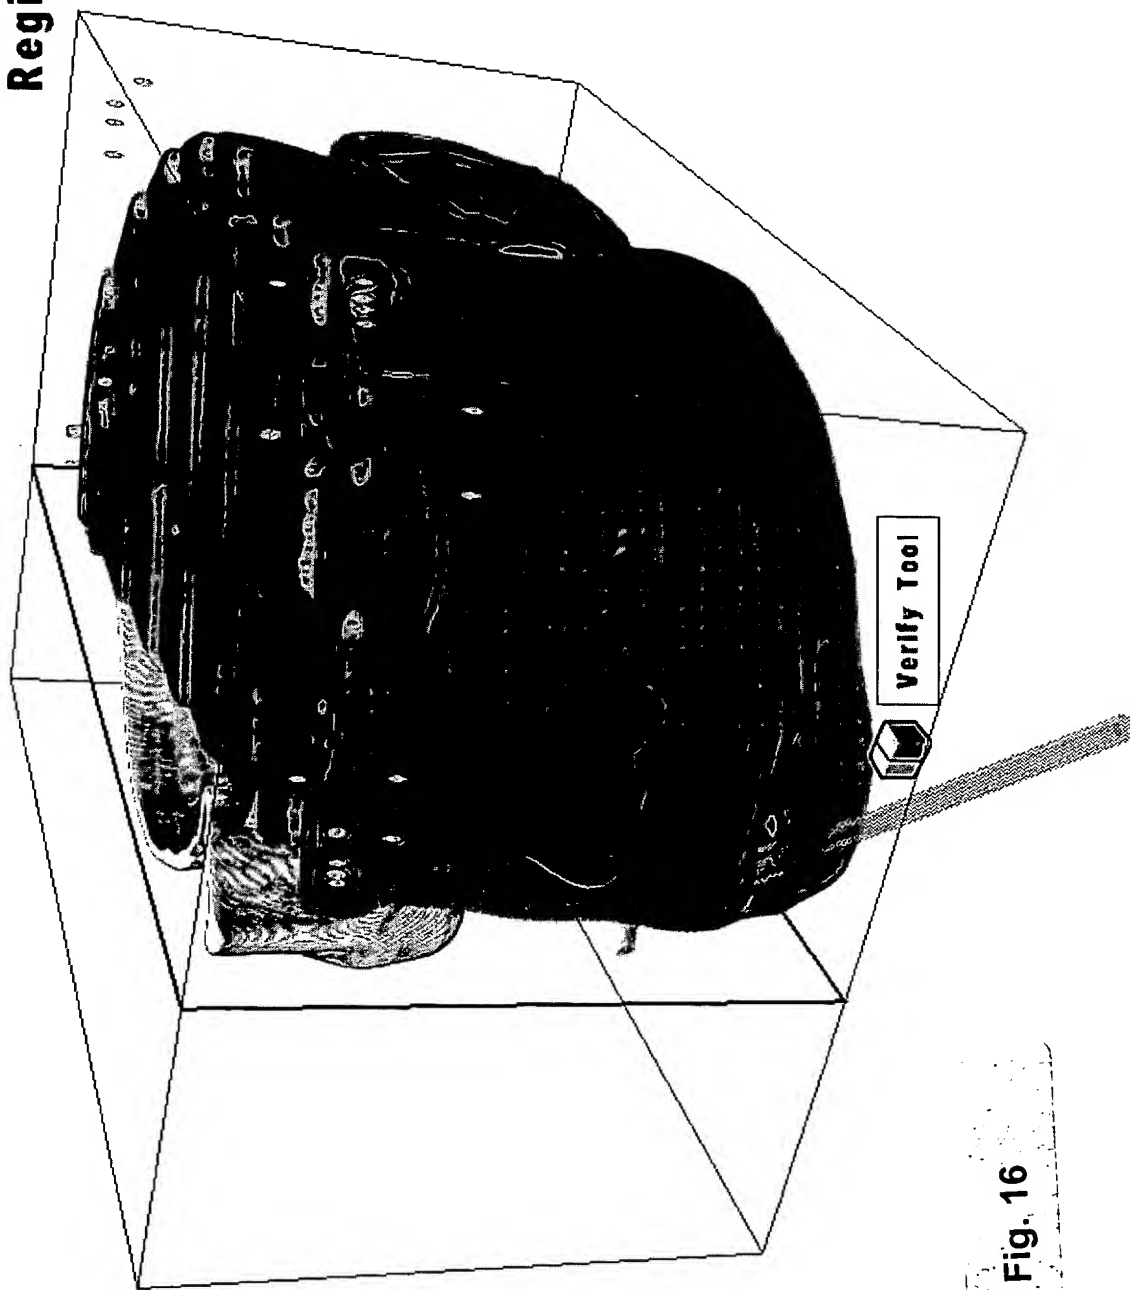


Fig. 16


ected object: MRI  
dality:  
e:  
ie:  
e: 256x256x52, 3.3MB

100  
100  
140  
100  
100  
20  
00  
40  
20  
0

Fig. 17




## Verify Registrati

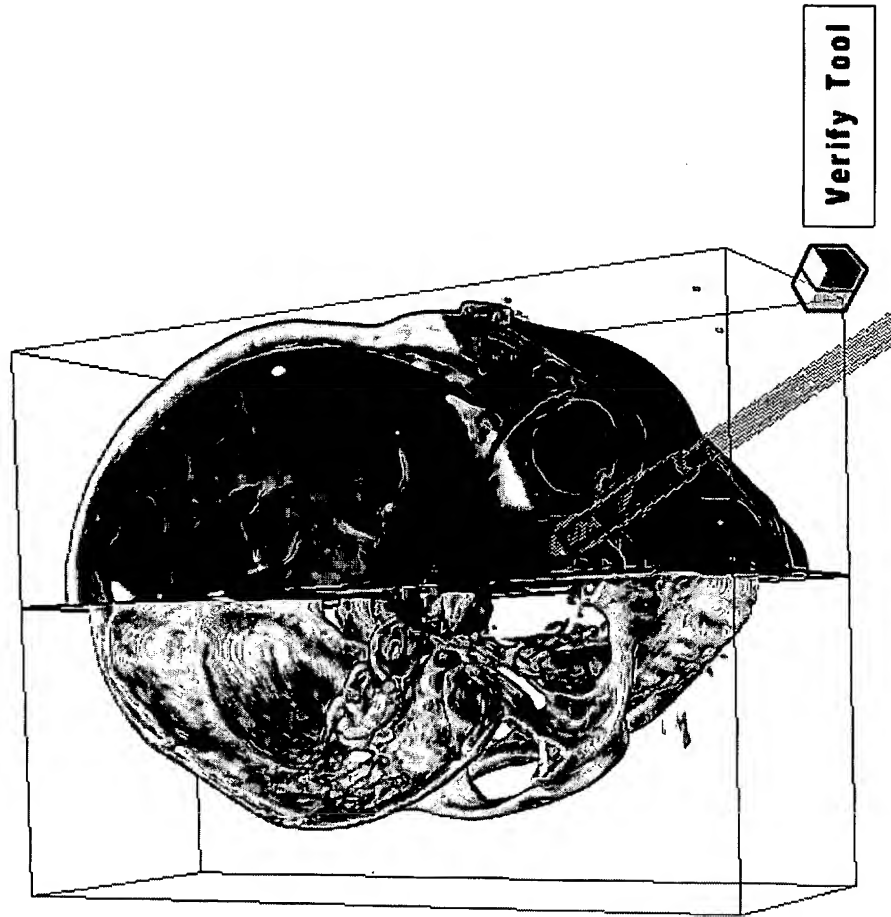

ected object: MRI  
dality:  
e:  
ie:  
e: 256x256x52, 3.3MB

Verify  
Registrati

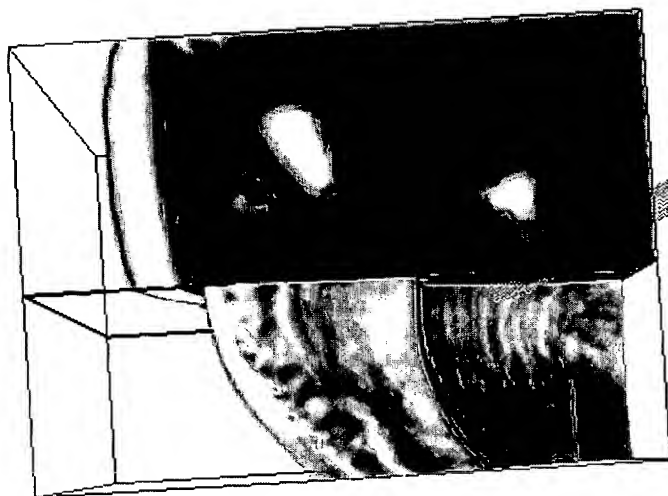

Verify Tool

Fig. 18

ected object: CT  
dality:  
e:  
e: 256x256x75, 4.7MB

# Verify 3D Registrati

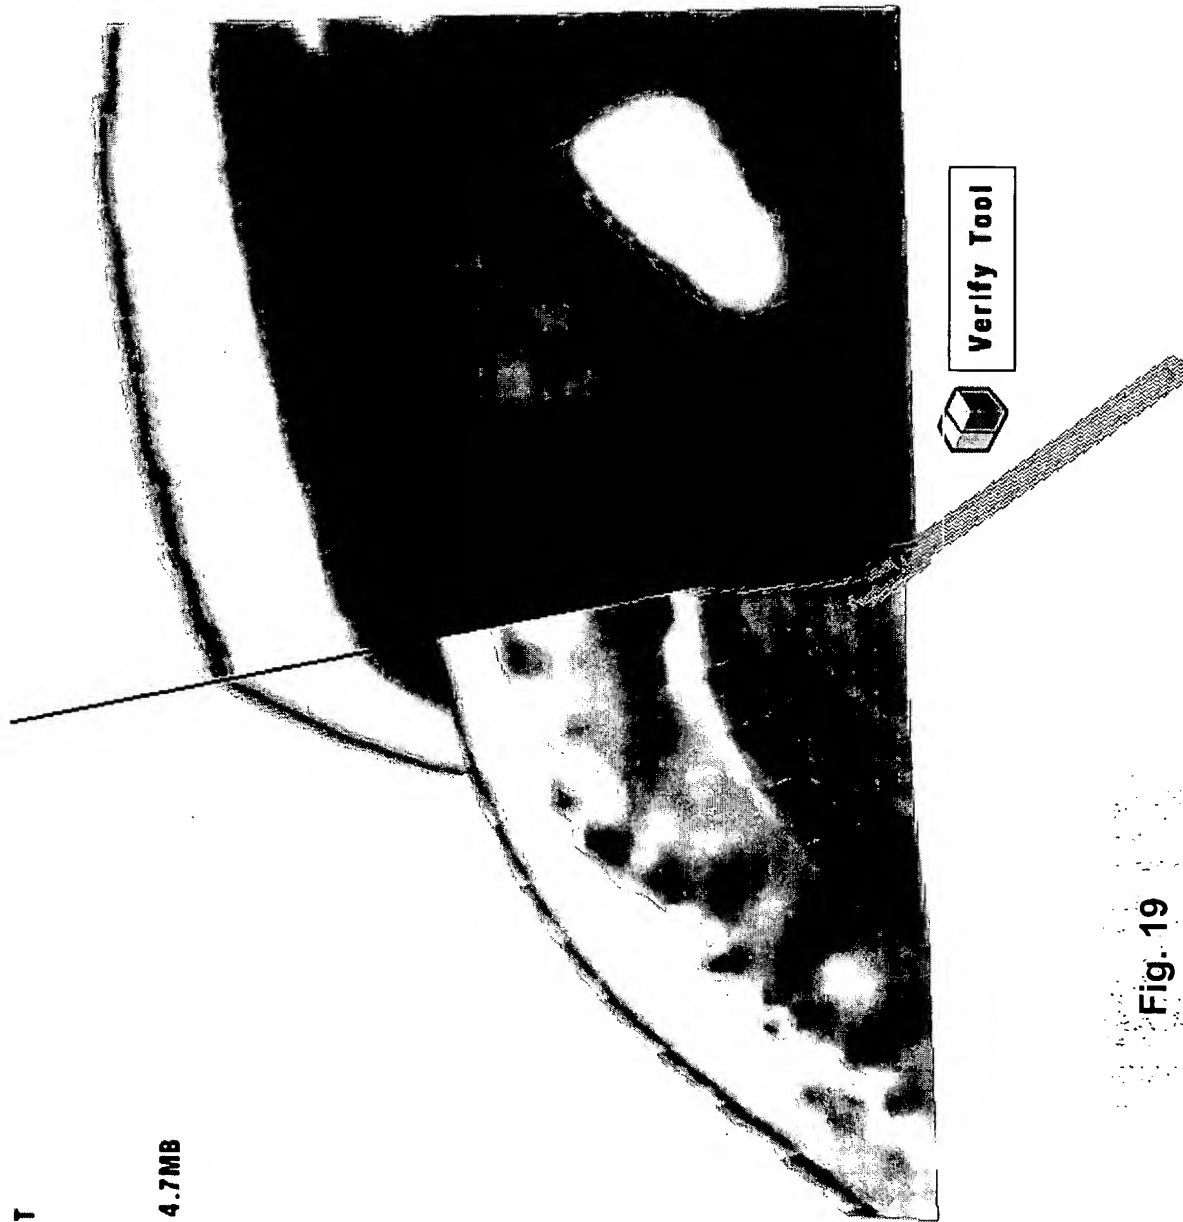



Fig. 19

ected object: CT  
 dality:  
 ie:  
 ie:  
 e: 256x256x75, 4.7MB

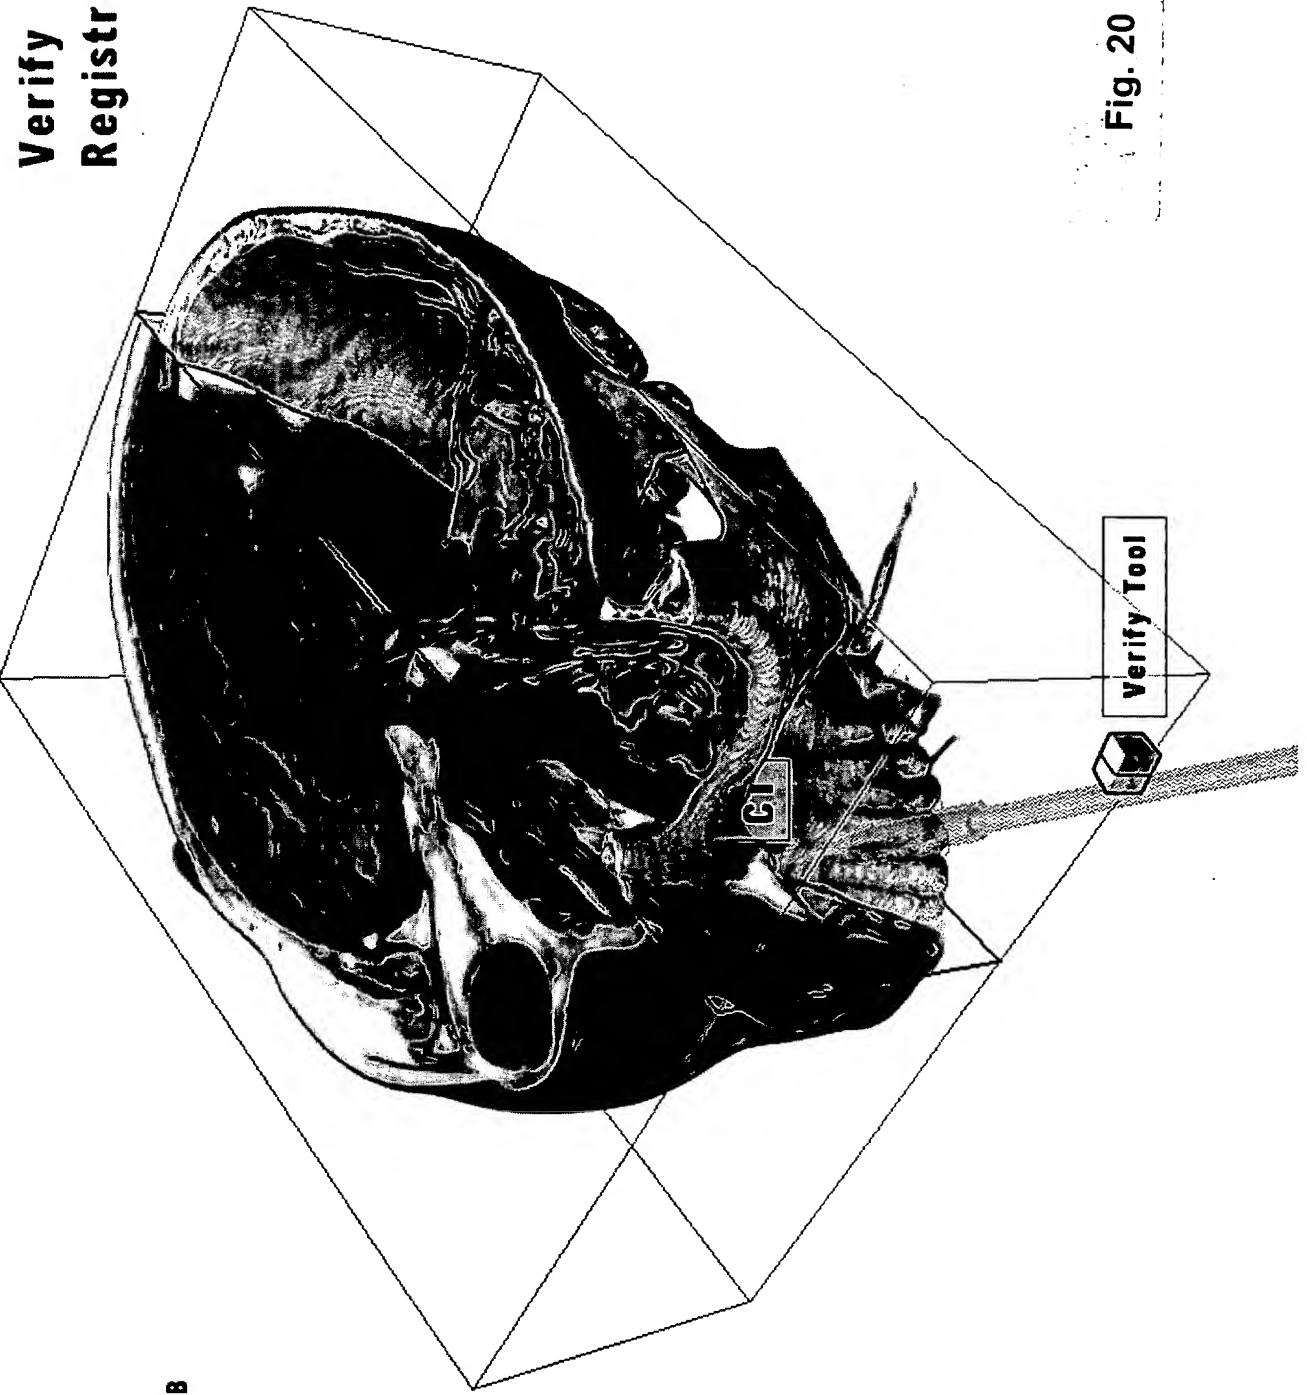


Fig. 20

ected object: CT

dality:

ie:

ie:

e: 256x256x75, 4.7MB

100  
20  
20  
70  
00  
20  
40  
30  
20  
10  
0

Fig. 21




Verify Tool




```
ected object: CT
dality:
e:
e:
e: 256x256x75, 4.7MB
```

## Verify Registrati

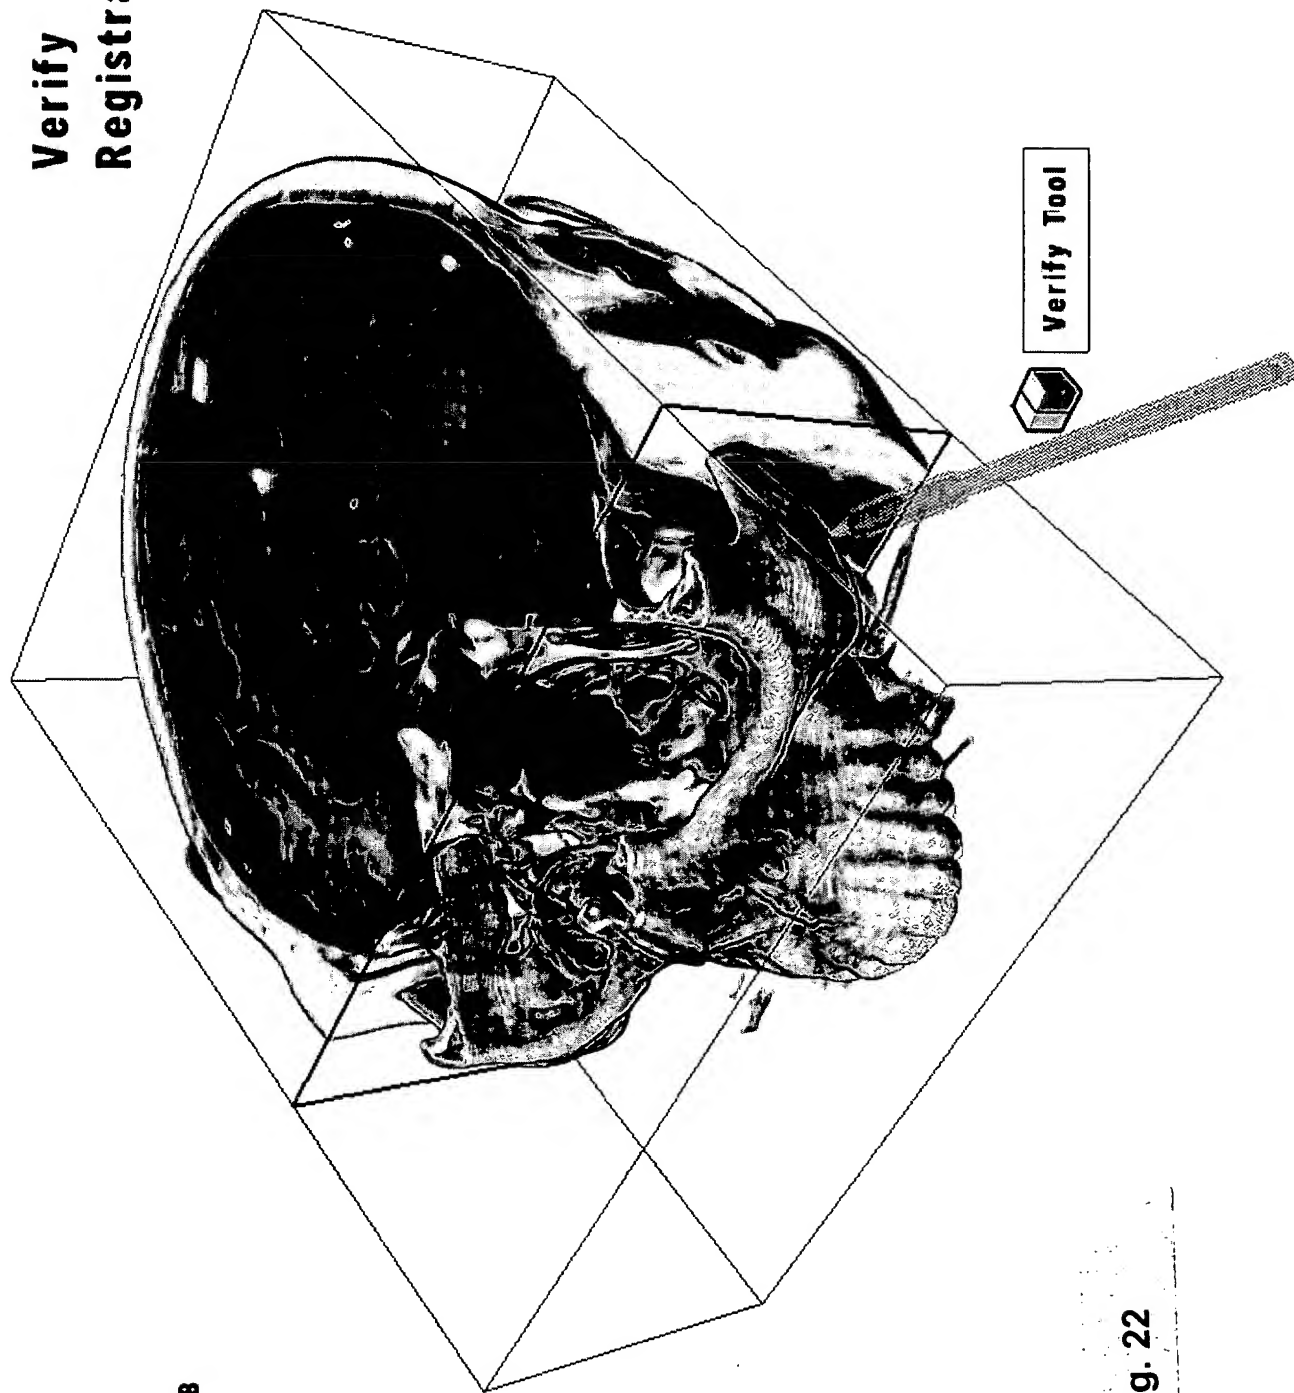

ected object: CT  
 dality:  
 :e:  
 ie:  
 e: 256x256x75, 4.7MB

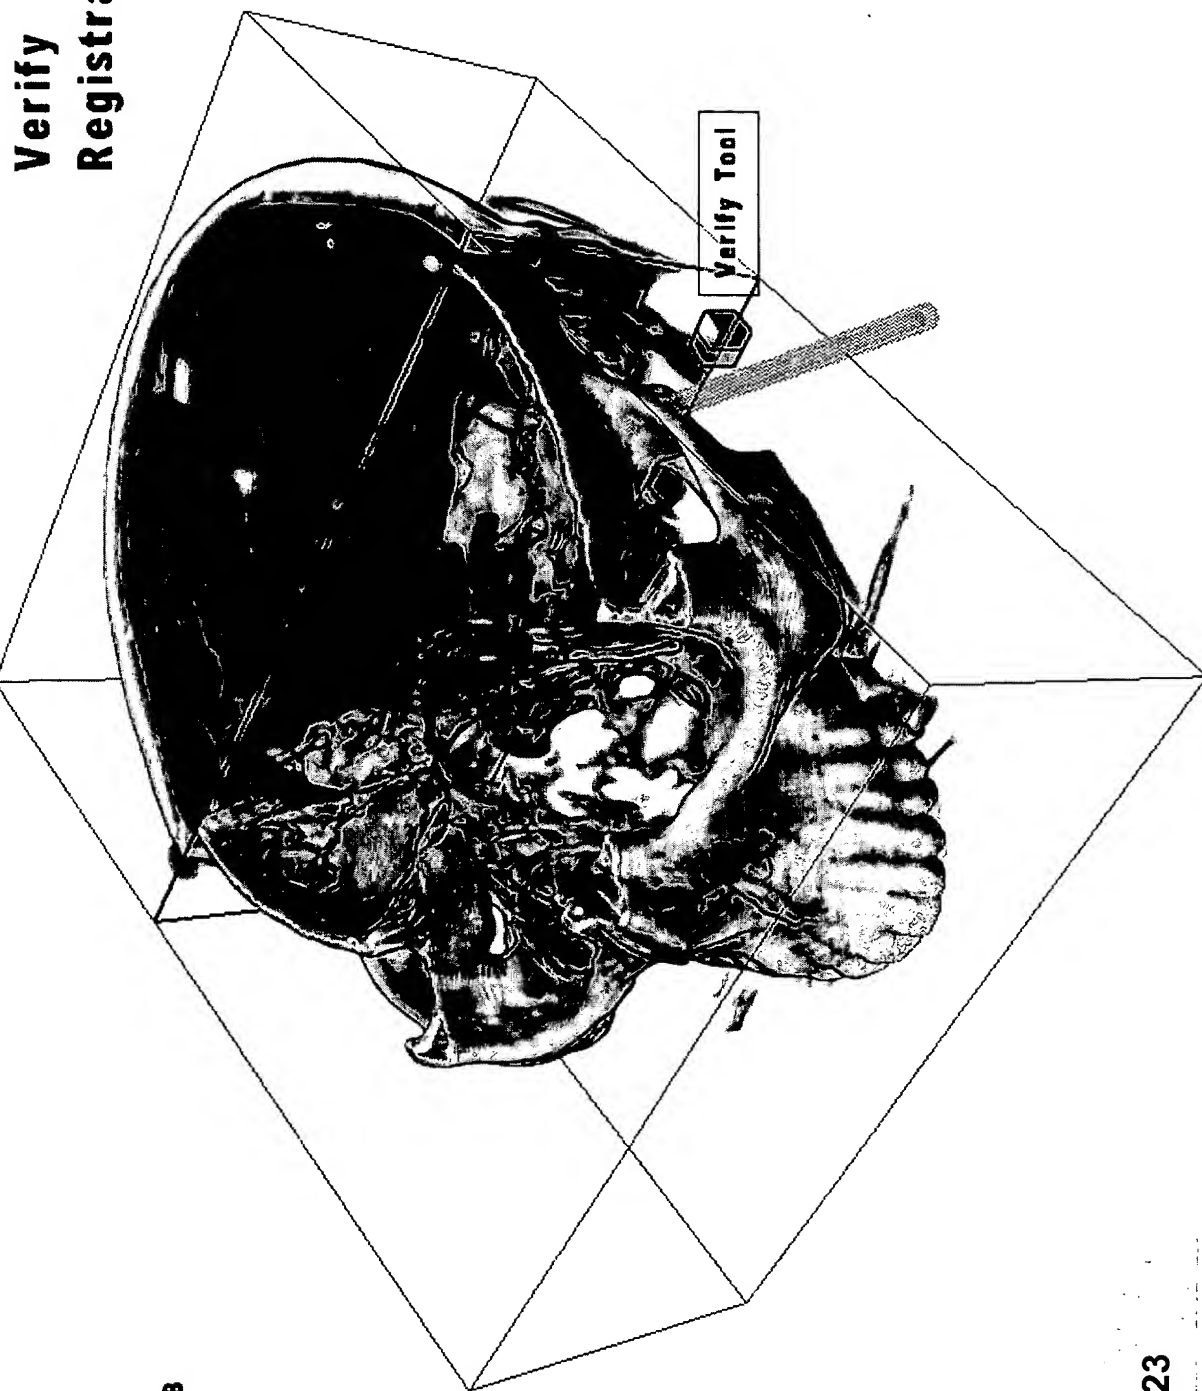

Verify  
 Registrati

Fig. 23

ected object: CT

dality:

ie:

ie:

e: 256x256x75, 4.7MB

# Verify Registrati


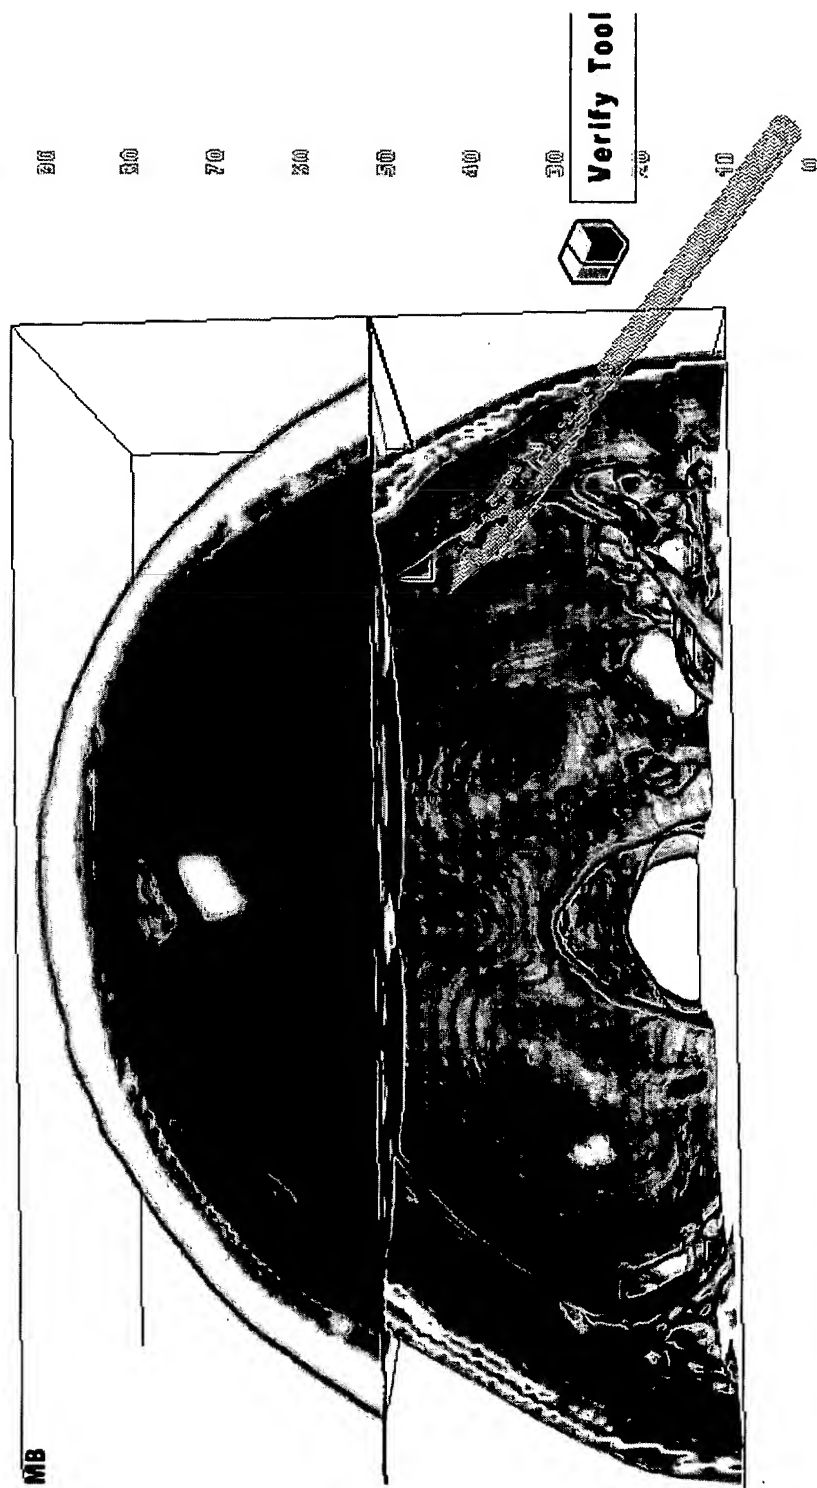


Fig. 24



# Verify Registrati

ected object: CT

dality:

ie:

ie:

e: 256x256x75, 4.7MB

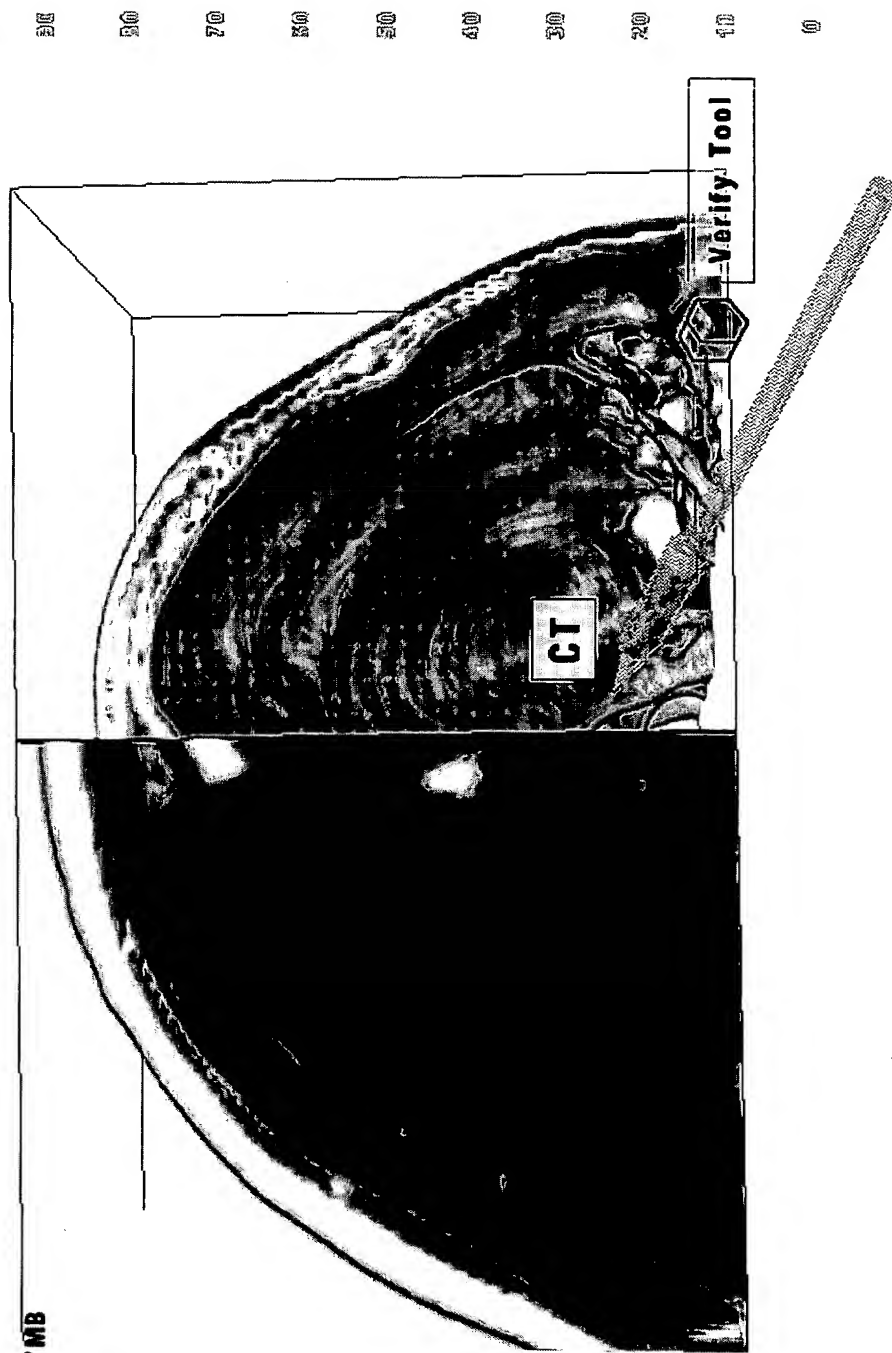


Fig. 25

ected object: CT

dality:

ie:

ie:


e: 256x256x75, 4.7MB



# Verify Registrati



Verify Tool



80  
60  
40  
20  
0

Fig. 26

ected object: CT  
 dality:  
 e:  
 e: 256x256x75, 4.7MB



# Verify Registrati

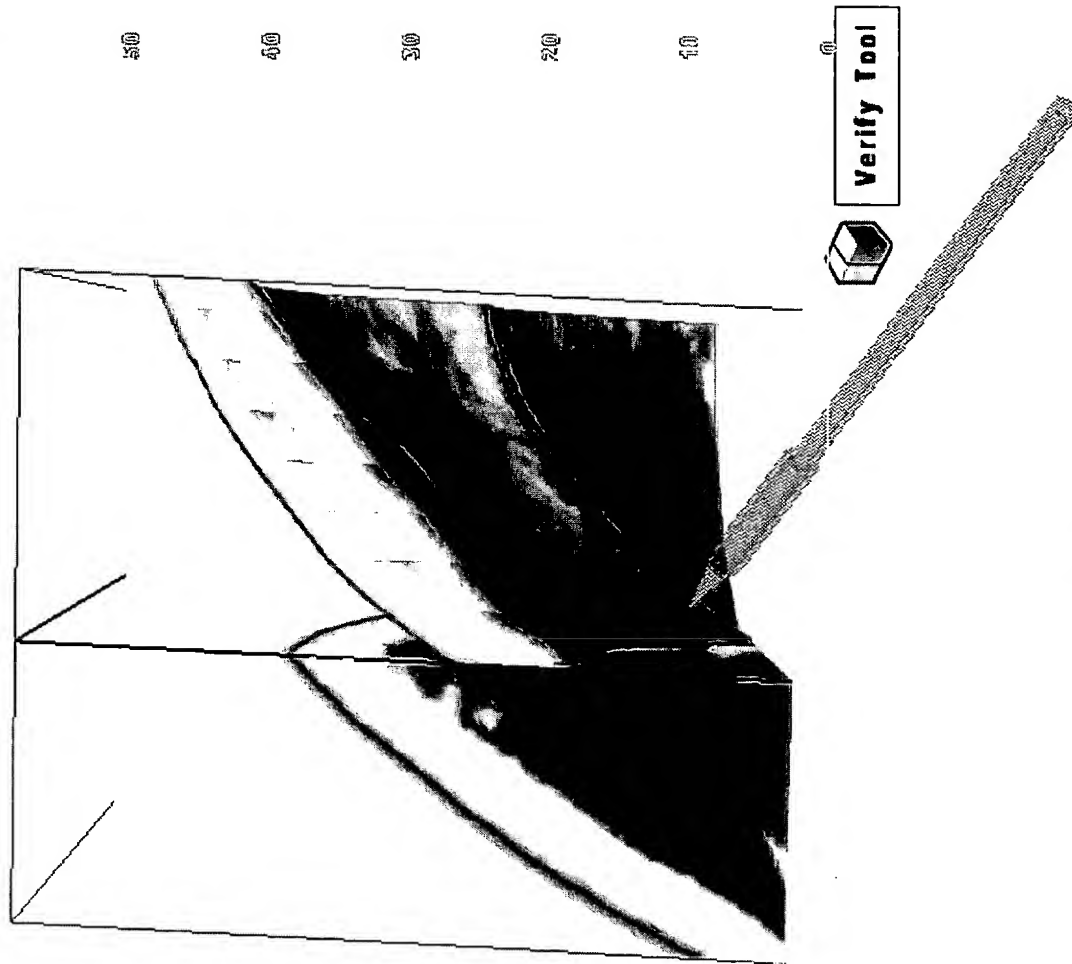


Fig. 27


ected object: CT

dality:

ie:

ie:

e: 256x256x75, 4.7MB



800

Verify

Registrati

800

800

800

800

800

800

800

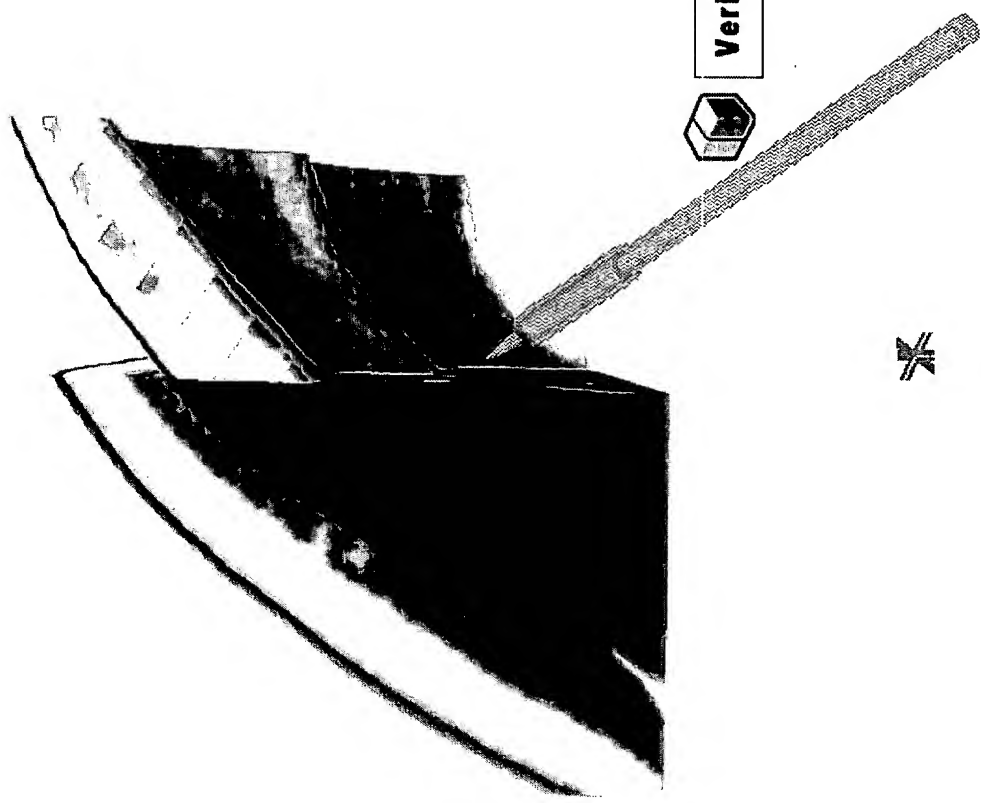


Fig. 28